JULY 15, 1928

PRICE LIST

X-RAY AND PHYSICAL-THERAPY **APPARATUS**

ACCESSORIES AND SUPPLIES




ALL PRICES ARE F. O. B. LYNN, MASS. and subject to change without notice Always order by Catalogue number and give full description. Cash discount quoted on request


CAMPBELL ELECTRIC MFG. CO.


Campbell Building 15-19 Stewart Street


LYNN, MASSACHUSETTS

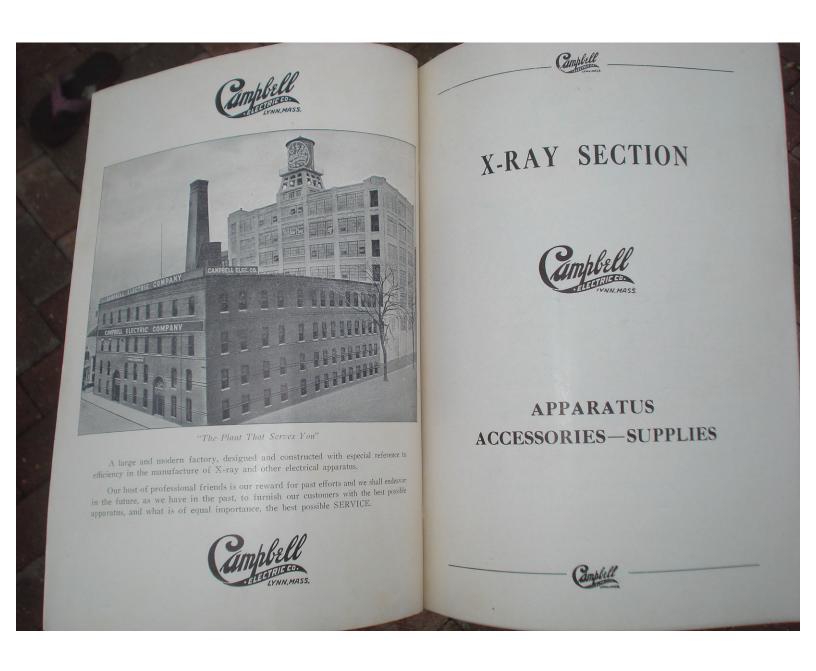





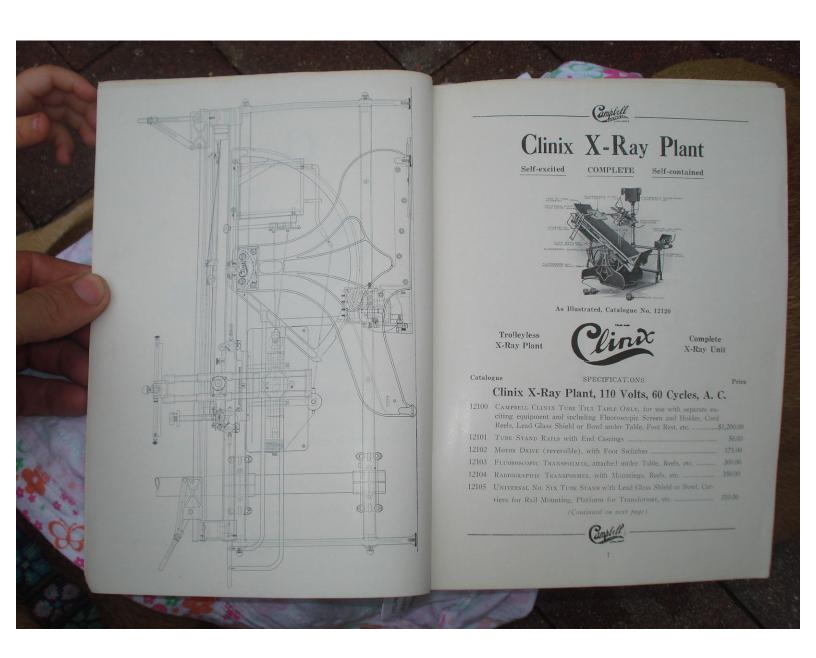


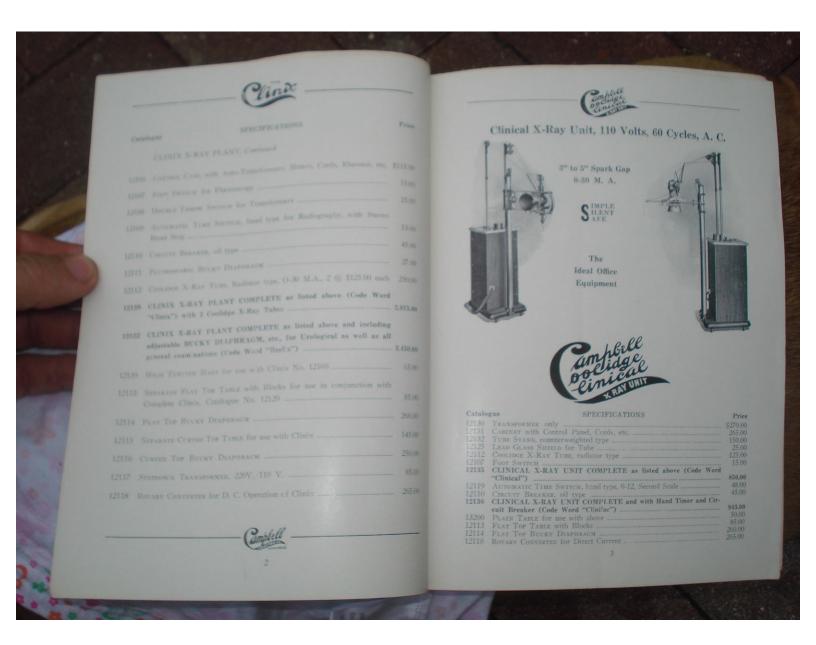

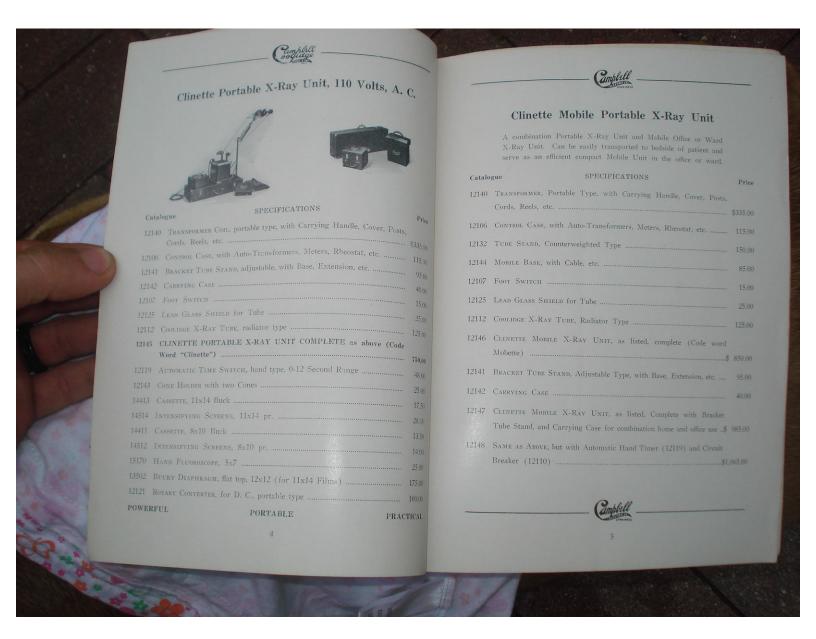

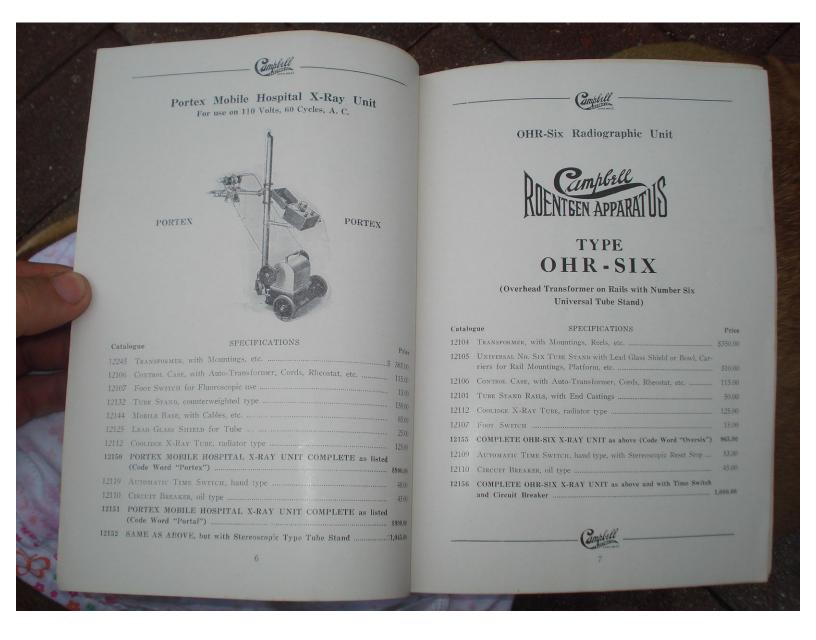

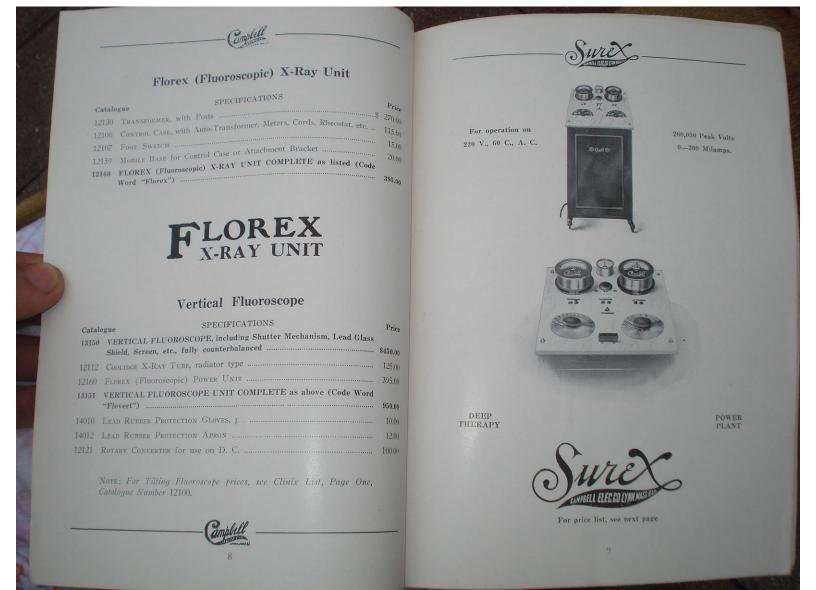

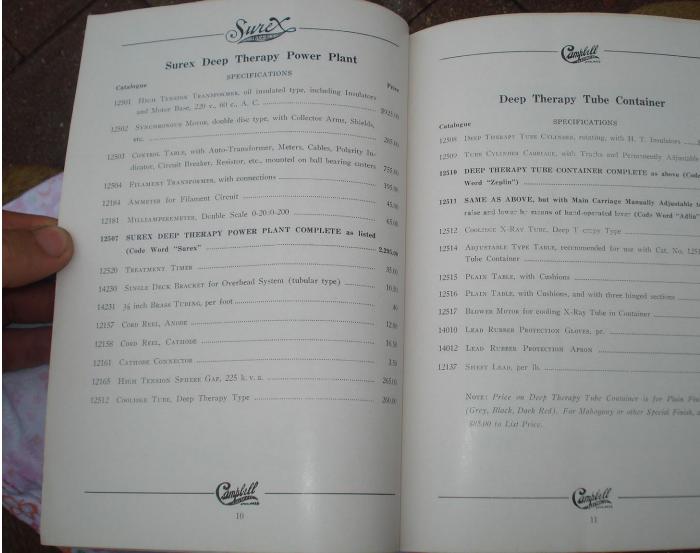


Deep Therapy Tube Container


Catalog	gue SPECIFICATIONS	Price
12508	DEEP THERAPY TUBE CYLINDER, rotating, with H. T. Insulators\$1	.060.00
12509	TUBE CYLINDER CARRIAGE, with Tracks and Permanently Adjustable	535.00
12510	DEEP THERAPY TUBE CONTAINER COMPLETE as above (Code	
	Word "Zeplin")	1 595 00
12511	SAME AS ABOVE, but with Main Carriage Manually Adjustable to	
	raise and lower by means of hand-operated lever (Code Word "Adlin")	1,945.00
12512	COOLIEGE X-RAY TUBE, Deep T erapy Type	
12514	ADJUSTABLE TYPE TABLE, recommended for use with Cat. No. 12510 Tube Container	225.00
12515	PLAIN TABLE, with Cushions	
12516	PLAIN TABLE, with Cushions, and with three hinged sections	. 225.00
12517	BLOWER MOTOR for cooling X-Ray Tube in Container	50.00
14010	LEAD RUBBER PROTECTION GLOVES, pr	. 10.00
14012	LEAD RUBBER PROTECTION APRON	. 12.00
12137	SHEET LEAD, per lb.	.85
	N. D. L. D.	


(Grey, Black, Dark Red). For Mahogany or other Special Finish, and



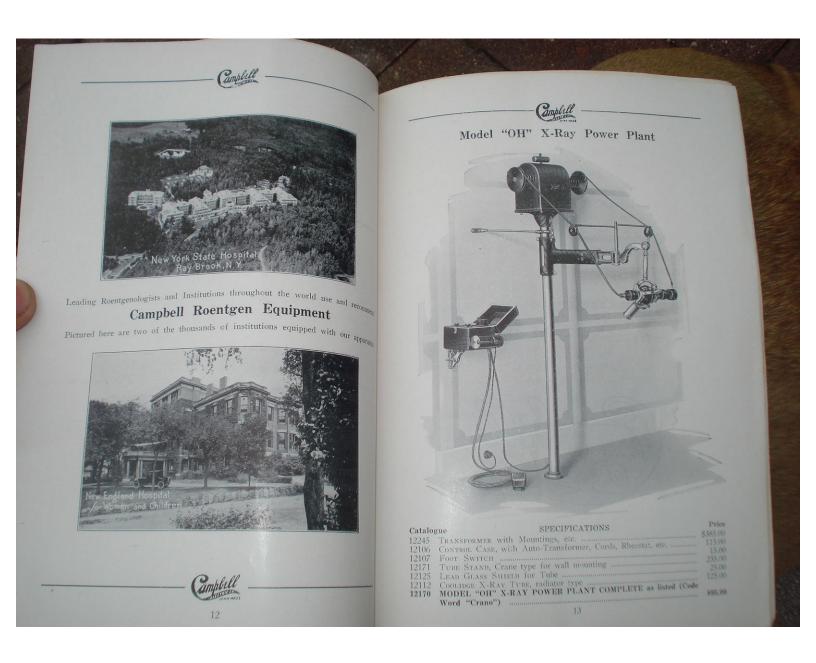



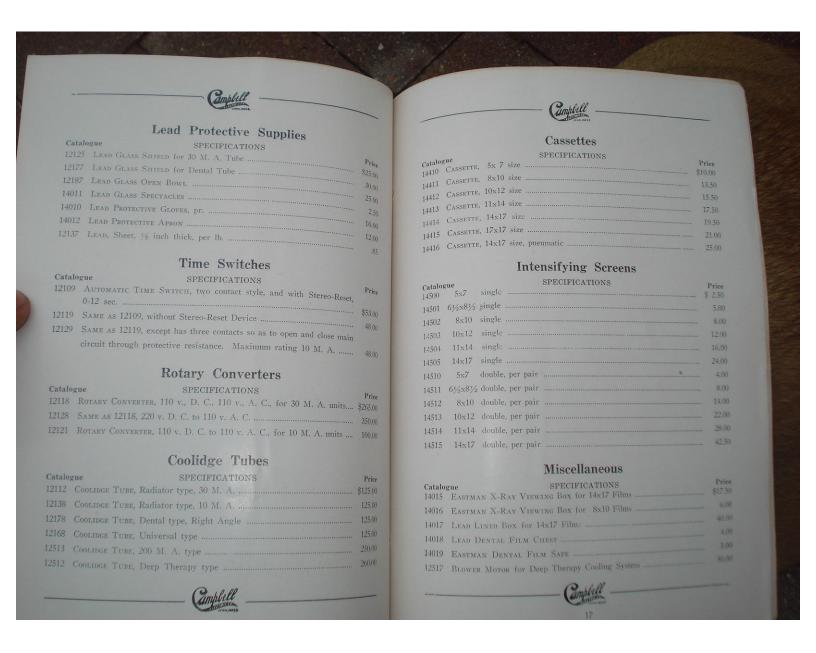

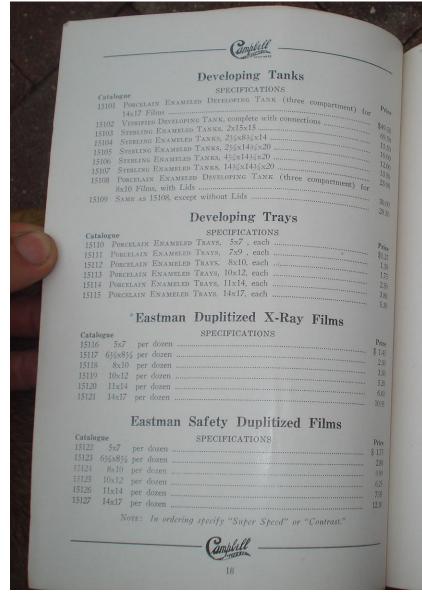





Eastman Dental X-Ray Films


SPECIFICATIONS

RADIATIZED "A", per package	Price
Regular (Non-Curling) "B", per package	\$1.15
Extra Fast (Non-Curling) "BB", per package	1.40
REGULAR "C", per package	1.40
Extra Fast "CC", per package	.70
BITE WING, Type 1, per package	.70
BITE WING, Type 3, per package	1.25
	1.75
Safelight Lamps	
Brownie Safelight Lamp	
	2 -110
	3.00
	3.50
Wratten, No. 2, without Slide	10.00
	8.00
X-Ray Developing Powders	
No. 2 package of six powders, sufficient to proper 12	
No. 3 package sufficient to prepare on - "	\$.60
No. 4 package sufficient to prepare five gallon ready to use solution	.83
prepare the gallons ready to use solution	3.50
X-Ray Fixing Powders	
No. 3—To make one gallon solution	
No. 4—To make five gallons solution	\$.60
g-section management and an arrangement and arrangement and arrangement and arrangement ar	2.50
X-Ray Film Hangers	
5×7	
(1) 0.1	\$.75
0½x8½	
6½x8½ 8x10	.85
8x10	1.25
8x10 10x12	1.25 1.50
8x10	1.25
	EXTRA FAST (Non-Curling) "BB", per package REGULAR "C", per package EXTRA FAST "CC", per package BITE WING, Type 1, per package BITE WING, Type 3, per package Safelight Lamps BROWNIE SAFELIGHT LAMP EASTMAN SAFELIGHT LAMP KODAK SAFELIGHT LAMP WRATTEN, No. 1, with Slide WRATTEN, No. 2, without Slide X-Ray Developing Powders No. 2 package of six powders, sufficient to prepare 12 oz. ready to use solution No. 3 package sufficient to prepare one gallon ready to use solution No. 4 package sufficient to prepare five gallons ready to use solution X-Ray Fixing Powders No. 3—To make one gallon solution No. 4—To make five gallons solution X-Ray Film Hangers




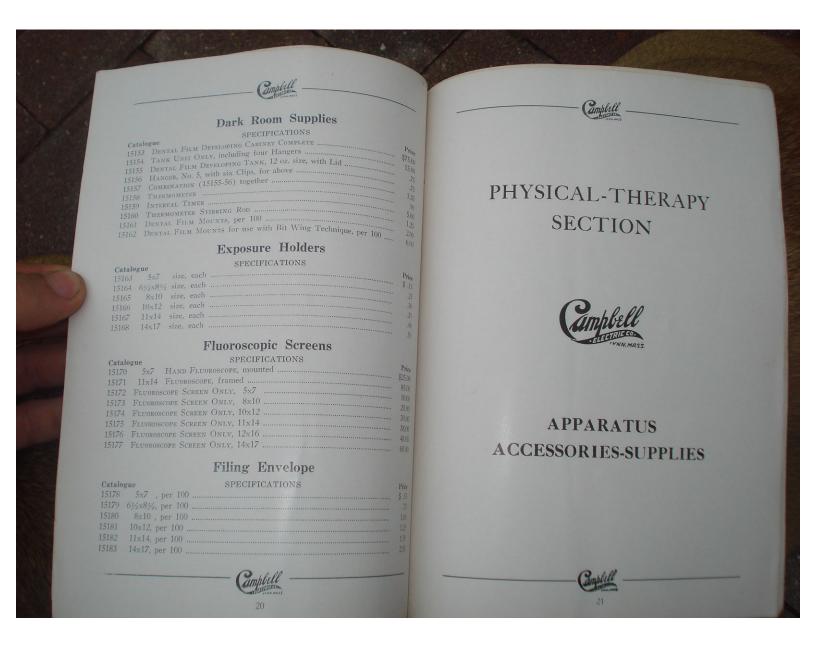


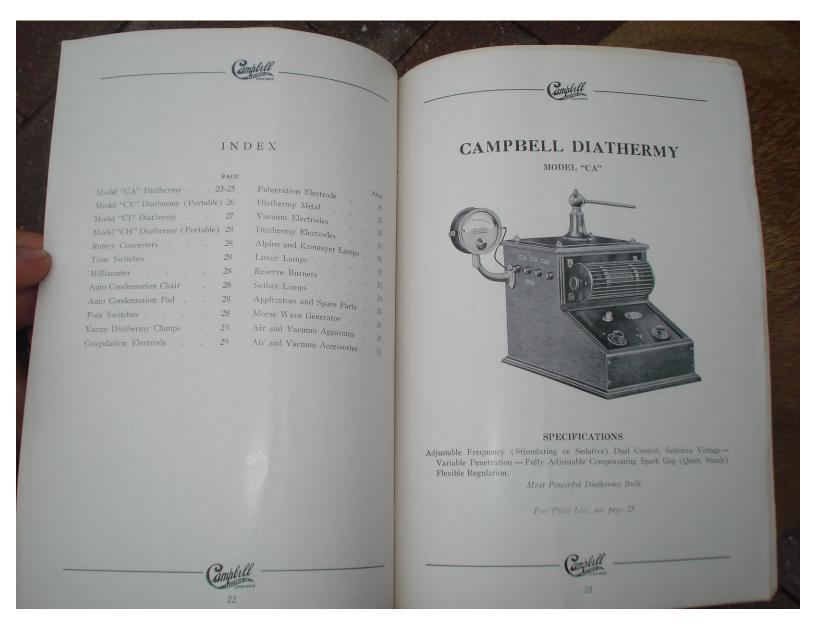

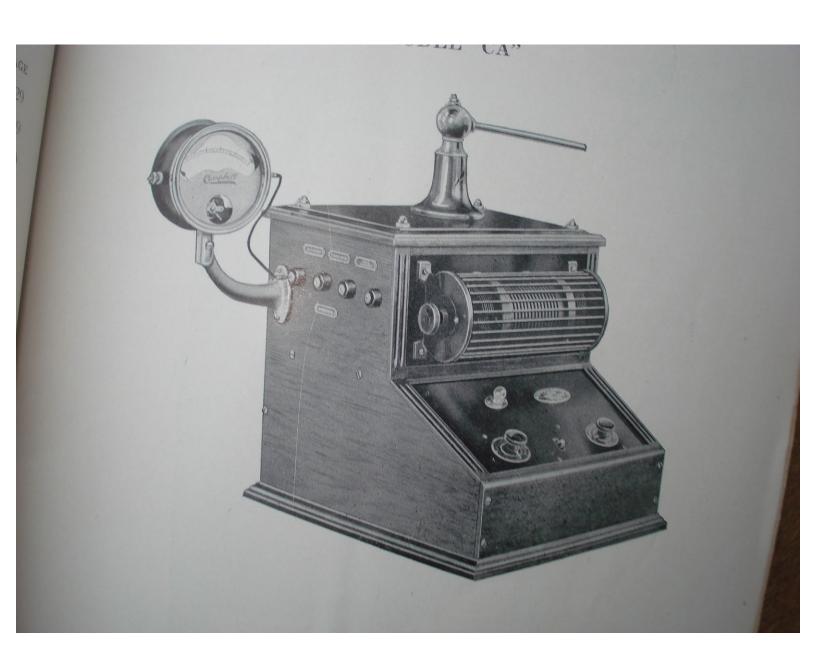



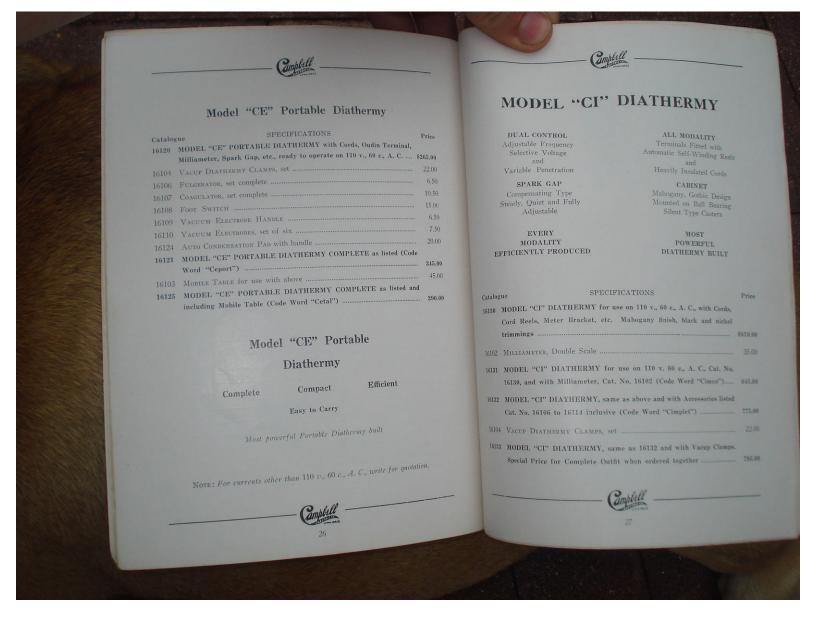

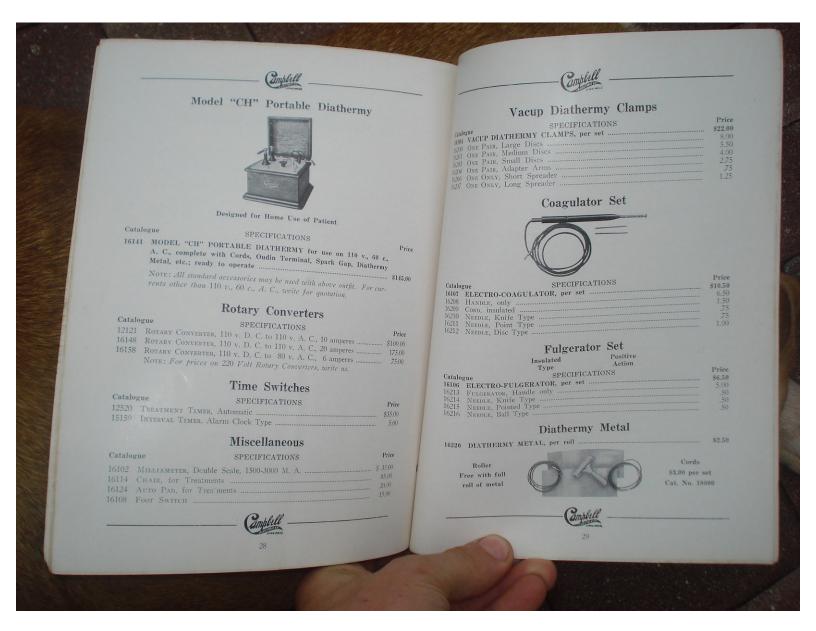



Model "CH" Portable Diathermy



Designed for Home Use of Patient


Price


alogue


SPECIFICATIONS


SPECIFICATIONS


for use on 110 v., 60 c.,

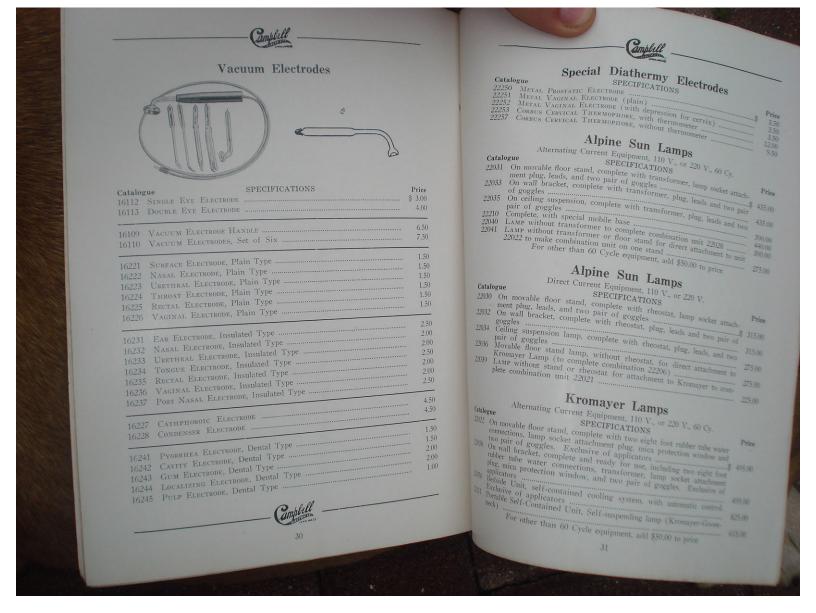

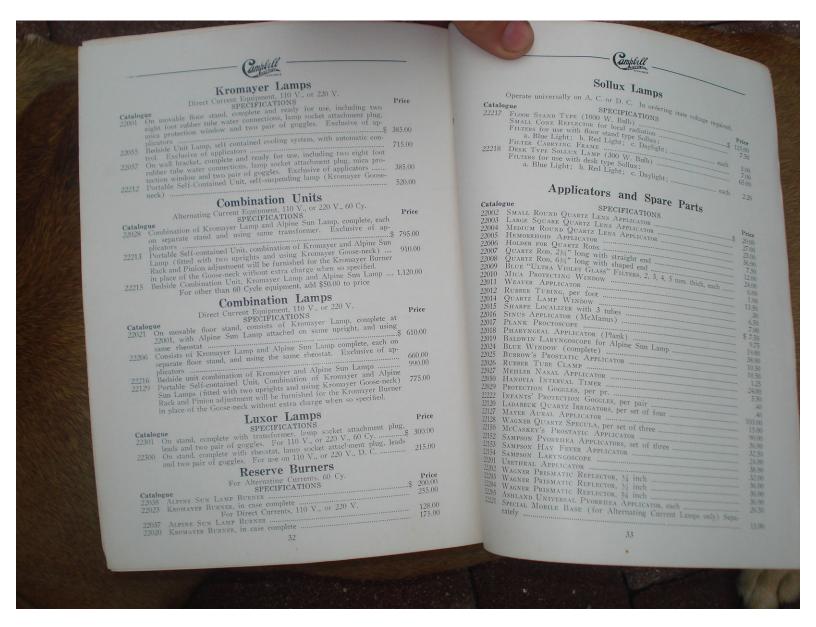

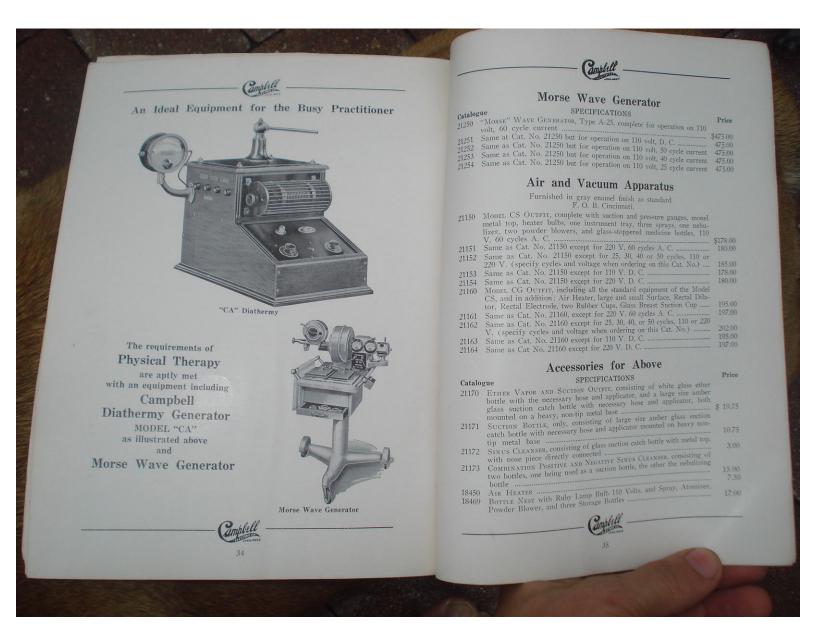

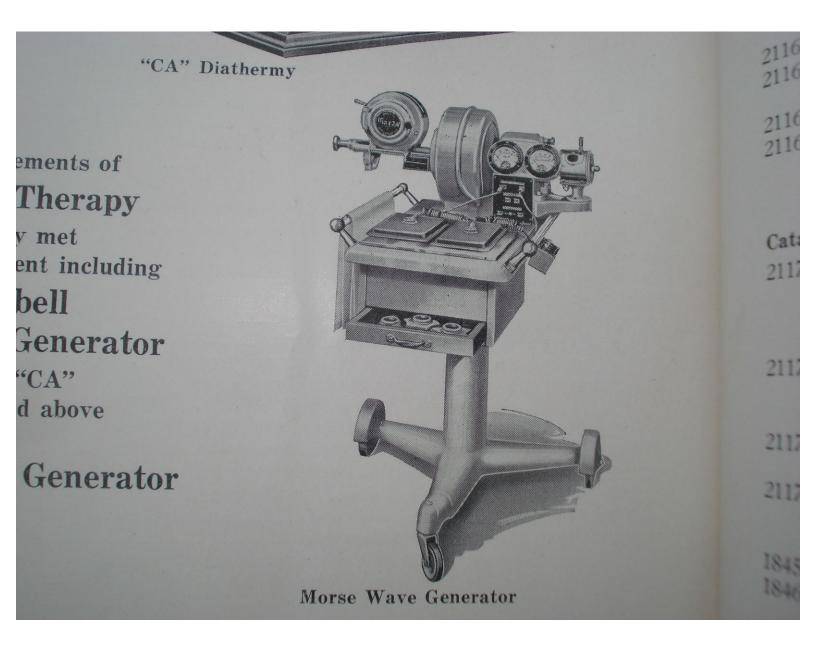

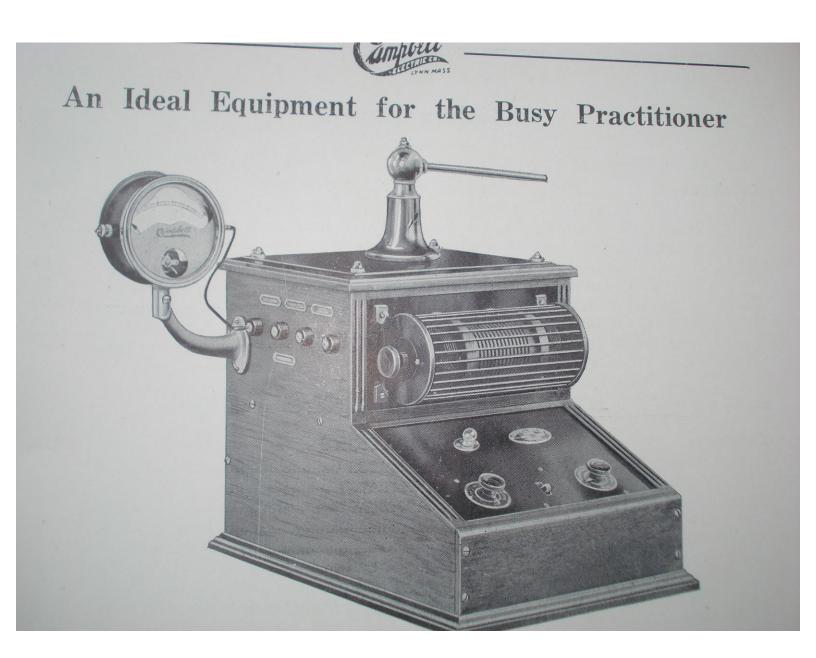



1898

1928

THIRTY YEARS OF PROGRESS WITH CAMPBELL



The first successful X-Ray and High Frequency Apparatus manufactured in the United States was built by CAMPBELL

Introduced to A. M. A. 1901

Ten years later thousands of improved types were giving service to the medical profession.





Steady and constructive progress by Campbell engineers, produced the perfected combination X-Ray and Electro-Medical equipment pictured to the left, many times copied but never equaled.

And now, in 1928, just thirty years since CAMPBELL produced the first Diathermy apparatus in the United States, there is available a complete line of efficient quality X-Ray equipment pictured on pages 1 to 14 inclusive of this booklet as well as four models of Diathermy apparatus (pages 23 to 28 inclusive), producing every modern modality radically in advance of anything yet offered. Send for catalogue.





Two Views of the Factory that Serves You



Screw Machines

SIX-FLOOR MODERN CEMENT BUILDING



A Corner of Our Machine Shop

TRAINED OPERATIVES OF LONG EXPERIENCE



